



FLOM UI-22 SERIES

Clarity Control Module

ENG

Code/Rev.: M232/100A

Date: 2026-02-25

Phone: +420 251 013 400

clarity@dataapex.com

www.dataapex.com

DataApex Ltd.
Petrzilkova 2583/13
158 00 Prague 5
Czech Republic

Clarity[®], DataApex[®] and ▲[®] are trademarks of DataApex Ltd. Microsoft[®] and Windows[™] are trademarks of Microsoft Corporation.
DataApex reserves the right to make changes to manuals without prior notice. Updated manuals can be downloaded from www.dataapex.com.

Author: KK

Contents

1 Flom UI-22 series and Flom UI-32 series Control Module	1
2 Requirements	2
3 Installation Procedure	3
3.1 Flom UI-22 series and Flom UI-32 series pump communication	3
3.2 Clarity Configuration	3
4 Using the control module	6
4.1 DataApex UNI Setup	6
4.2 Method Setup - LC Gradient	7
4.2.1 Gradient Options	10
4.3 Method Setup - LC	11
4.3.1 Hardware Configuration	12
4.4 Method Setup - Event Table	12
4.5 Method Setup - Aux. Signals	13
4.6 Device Monitor	14
4.6.1 LC Control Manual Flow	16
5 Report Setup	18
6 Troubleshooting	19

To facilitate the orientation in the **Flom UI-22 series** manual and **Clarity** chromatography station, different fonts are used throughout the manual. Meanings of these fonts are:

Open File (italics) describes the commands and names of fields in **Clarity**, parameters that can be entered into them or a window or dialog name.

WORK1 (capitals) indicates the name of the file and/or directory.

ACTIVE (capital italics) marks the state of the station or its part.

Chromatogram (blue underlined) marks clickable links referring to related chapters.

The bold text is sometimes also used for important parts of the text and the name of the **Clarity** station. Moreover, some sections are written in format other than normal text. These sections are formatted as follows:

Note: Notifies the reader of relevant information.

Caution: Warns the user of possibly dangerous or very important information.

█ Marks the problem statement or trouble question.

Description: Presents more detailed information on the problem, describes its causes, etc.

Solution: Marks the response to the question, presents a procedure how to remove it.

1 Flom UI-22 series and Flom UI-32 series Control Module

This manual describes the set up of the **Flom UI-22 series** and **Flom UI-32 series** pumps. The control module enables direct control of the instrument.



Fig. 1: Flom UI-22 series pump

Direct control means that the pump can be completely controlled from the Clarity environment. The Instrument method, controlling the analysis conditions, will be saved in the measured chromatograms.

The control is performed via the **UNI Ruby** control module and the **Flom UI-22 series** script.

2 Requirements

- Clarity installation with LC Control module (p/n A24).
- Free serial COM port in the PC.

Note: Modern computers usually have only one (if any) serial (COM) port installed. To use more devices requiring the RS232 port, the MultiCOM adapter (p/n MC01) is available.

- Serial DB9F-DB9F cross cable (p/n SK01).

Note: Cables are not part of Clarity Control Module. It is strongly recommended that you order the required cables together with the software.

3 Installation Procedure

3.1 Flom UI-22 series and Flom UI-32 series pump communication

The **Flom UI-22 series** and **Flom UI-32 series** is controlled by serial (RS232) communication.

It uses a standard serial DB9F-DB9F cross cable (p/n SK01) described in the picture below.




Fig. 2: Serial DB9F-DB9F cross

3.2 Clarity Configuration

The following section provides step-by-step guide on how to configure the UI-22 or UI-32 pump to be used in Clarity.

- Start Clarity.
- Invoke the dialog from the **Clarity** main window using the **System - Configuration...** command.
- Press the **Add** button (ⓘ on **Fig. 3** on pg. 4.) to invoke the **Available Control Modules** dialog.

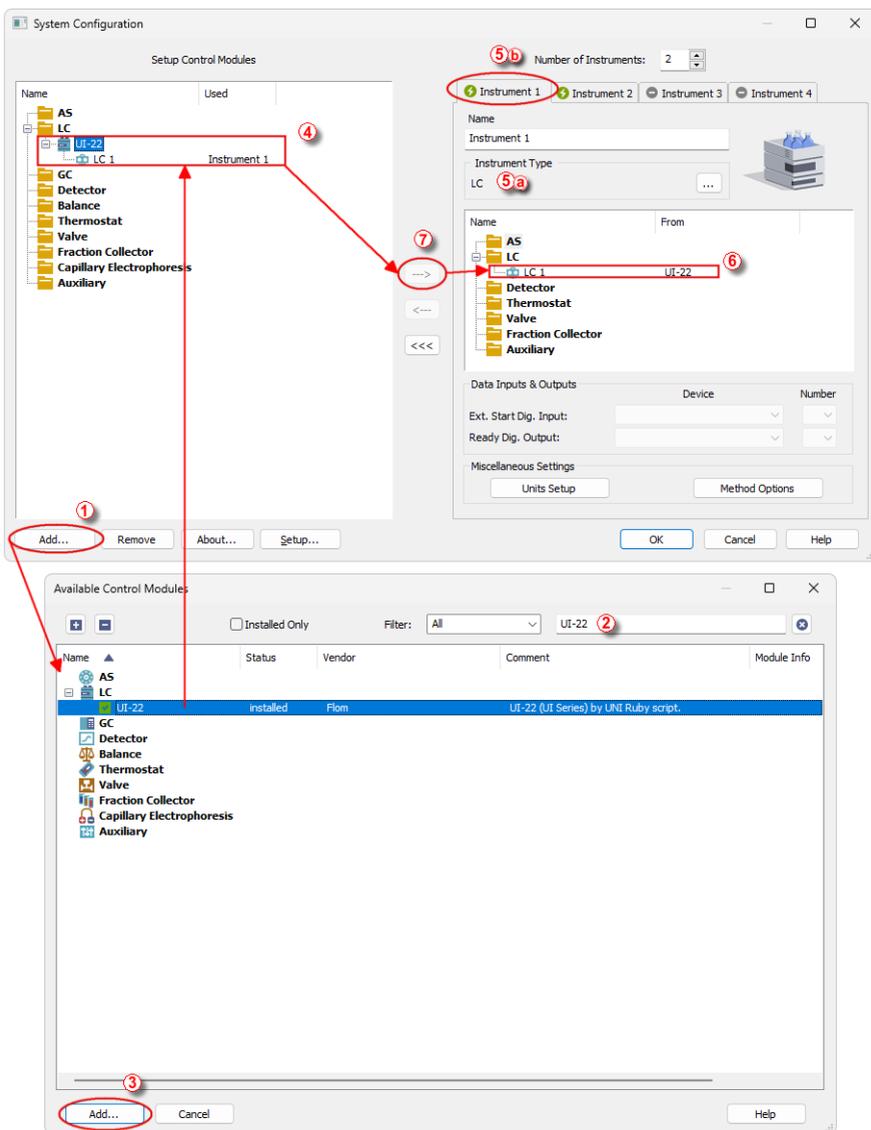


Fig. 3: How to Add Flom pumps module

- You can specify the search filter ② to simplify the finding of the driver.
- Select the correct item and press the *Add* (③ on **Fig. 3** on pg. 4.) button. Each device with already created UNI profile should have its own item named accordingly in the *Available Control Modules* dialog.

- The *DataApex UNI Setup* dialog will appear.

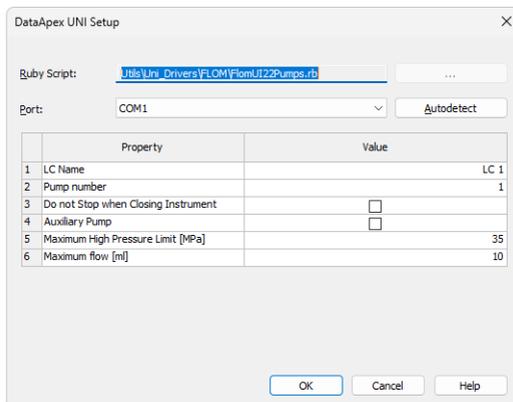


Fig. 4: DataApex UNI Setup

- Set the correct communication *Port* and click on the *Autodetect* button to establish communication with the device.
- You may fill in the custom *LC Name* and other custom settings. The *DataApex UNI Setup* dialog is described in detail in the chapter "**DataApex UNI Setup**" on pg. 6.
- The **Flom UI-22 series** or **Flom UI-32 series** item ④ will appear in the *Setup Control Modules* list of the *System Configuration* dialog.
- Change the *Instrument Type* ⑤ ⑧ on the desired *Instrument* tab ⑤ ⑥ to LC.
- Drag the appropriate item from the *Setup Control Modules* list on the left ④ to the *Instrument* tab on the right ⑥ , or use the button ⑦ .

4 Using the control module

After adding and setting up the new device one or more new tabs will appear in the *Method Setup* dialog depending on the type of the instrument. A new **Flom UI-22 series** or **Flom UI-32 series** pump section enabling the monitoring of the current pump state will be also created in the *Device Monitor* window.

4.1 DataApex UNI Setup

The *DataApex UNI Setup* dialog defines the connection to the pump and sets the basic pump limits and behavior.

	Property	Value
1	LC Name	LC 1
2	Pump number	1
3	Do not Stop when Closing Instrument	<input type="checkbox"/>
4	Auxiliary Pump	<input type="checkbox"/>
5	Maximum High Pressure Limit [MPa]	35
6	Maximum flow [ml]	10

Fig. 5: DataApex UNI Setup

Note: The pump subtype is not auto-detected, so the flow and pressure limits must be set manually according to the pump subtype and pump head used. Flow and pressure limits are listed in the table below.

Tab. 1: Pressure and flow limits

Pump Subtype	Flow limit	Pressure limit
UI-22-110P	0.001 - 9.999 ml/min	20 MPa
UI-22-110S	0.001 - 9.999 ml/min	35 MPa
UI-22-410S	0.01 - 99.99 ml/min	5 MPa
UI-32-110P	0.001 - 9.999 ml/min	20 MPa
UI-32-110S	0.001 - 9.999 ml/min	40 MPa
UI-32-410P	0.01 - 99.99 ml/min	5 MPa
UI-32-410S	0.01 - 99.99 ml/min	5 MPa

Ruby Script

Displays the selected Ruby Script. The correct FLOMUI22PUMPS.RB script for the **Flom UI-22 series** or **Flom UI-32 series** instrument can be found in the UTILS/UNI_

DRIVERS/FLOM subdirectory (accessible through the button) of the Clarity installation folder (C:\CLARITY\BIN by default).

Port

Defines the communication port used, possible values dependent on the type of communication of the device and/or available ports in the PC.

AutoDetect

It is used for verifying the device communication over the serial port selected above.

Instrument Name

Allows you to set the custom name of the instrument. This name (entered into the *Value* column) will be used throughout the Clarity station.

Pump Number

Here you can set the number corresponding to the selected pump (from 0 to 9).

Do not Stop when Closing Instrument

The pumps will not be shut down when closing the Clarity Instrument if this option is ticked.

Auxiliary Pump

The selected pump will be set as an auxiliary pump when ticking this box.

Maximum High Pressure Limit [MPa].

It sets a limit to the High Pressure value set on the Method.

Maximum Flow [ml].

It sets a limit to the Maximum Flow value set on the Method.

4.2 Method Setup - LC Gradient

The *Method Setup - LC Gradient* tab is used for preparing and editing the instrument method used by the **Flom UI-22 series** or **Flom UI-32 series** pump.

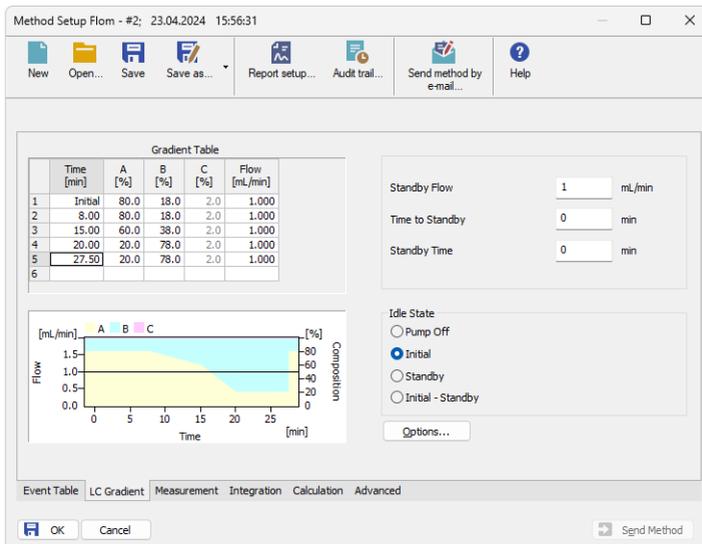


Fig. 6: Method Setup - LC Gradient

Gradient Table

A table for setting the composition of the mobile phase and the overall flow rate as a function of time. Operation is analogous to that of spreadsheets (Excel, Quatro Pro, etc.). To prepare the cell to receive values, click it by the left mouse button; the cell will highlight by dots. A cell that fails to highlight is not available for editing.

Time [min.]

Sets the time at which the ratio of flow rates and the overall flow rate correspond to the values entered in the corresponding row. (These values vary continuously from one time to the next in a manner ensuring that the conditions specified in the next row are satisfied).

XXX1 (.4) [%]

Represents the percentage of a component. The designation **XXX1-4** is in fact replaced by the name of the component (items *Solvent 1 - 4* in the **Gradient Options** dialog). Should you enter a component value such that the sum of all values exceeds 100 %, the percentage in the last column is automatically adjusted; if the percentage of the last compound is already zero, the value of the currently entered component is adjusted instead. The flow rate of a compound is calculated by multiplying the overall flow rate (indicated in the *Flow* column) by the corresponding percentage divided by 100.

Flow [ml/min]

Indicates the overall flow rate through the column. The entered value applies to the time specified in the corresponding row. The range for *Flow* values is 0 - 5 ml/min.

Graph

The graph depicts the percentage of components as a function of time together with the overall flow rate. Data are taken over from the *Gradient Table*. Changes effected in this table are immediately reflected in the graph. Legend in the header of the graph indicates the assignment of colors to individual components. The assignment is fixed and individual components are displayed in the graph from bottom to top. The flow rate is displayed as a black line.

The graph has two vertical axes: the axis on the left refers to the overall flow rate, the one on the right to the mixing ratio.

Parameters

Standby Flow

Sets the overall flow rate through the column in the *STANDBY* state reached after the last row of the table has been performed and the time period defined in the *Time to Standby* field has passed. The duration of this state is defined by the *Standby Time* item. The ratio of individual components in the respective *STANDBY* and *IDLE* states is given by the first row of the *Gradient Table* (the *Initial* row).

Time to Standby [min]

Indicates the time during which the flow rate and mobile phase composition changes continuously between the last values entered in the table and the values defined by *Standby Flow* field and the *Initial* row mobile phase composition.

This time is included in the analysis time (the Instrument is in the *CONTROL* state). In case when the *Time to Standby* is zero, there is step change from flow and components percentage specified on the last row of gradient table to that specified for *STANDBY* state.

Standby Time [min]

The time during which the flow rate is maintained at *Standby Flow*. This time is included in the analysis time (the Instrument is in the *CONTROL* state).

Idle State

An item specifying the overall flow rate through the column outside the instrument method. The following options are possible:

Pump Off

The flow rates of all components are zero.

Caution: Be careful as this setting may damage the column in some cases.

Initial

The flow rate is defined by the first row of the gradient table (the *Initial* row).

Standby

The flow rate is the same as in the *STANDBY* mode and, accordingly, corresponds to the value entered in *Standby Flow* field.

Initial - Standby

The flow is defined by the first row of the gradient table (the *Initial* row) after the method is sent, or by the value entered in the *Standby Flow* field after the method finishes.

The *IDLE* state comes into effect each time an Instrument is opened, at the end or after abortion of an analysis by the *Abort* command, and is also maintained after the Clarity program is shut down.

The mixing ratio of individual components in both the *IDLE* and *STANDBY* states is given by the first row of the *Gradient Table* (the *Initial* row).

Note: There is a step change in the flow and components percentage from the values specified for the *STANDBY* state to those specified for the *IDLE* state if the *Idle State* field is not set to *Standby*.

4.2.1 Gradient Options

Invoke the *Options...* button in the *Method Setup - LC Gradient* dialog to open the *Gradient Options* dialog. This dialog allows to set the custom name for particular solvents, to switch whether they are used or not in the gradient and to set the warning levels for pressure to prevent the damage to hardware.

Fig. 7: Gradient Options

Min. Pressure

Sets the minimum pressure for the given pump. When pressure drops to the set value, the pump will shut down. This prevents the solvent leakage. The range for *Min. Pressure* values is dependent on the pump variant and used pump head.

Max. Pressure

Sets the maximum pressure for the given pump. When pressure reaches the set value, the pump will shut down. This serves to prevent the damage to the pump when the column is blocked. The range for *Max. Pressure* values is dependent on the pump variant and used pump head and is limited by the value set for the pressure in the [DataApex UNI Setup](#) dialog. *Max. Pressure* must also be at least 1 MPa higher than the *Min. Pressure*.

Note: Pressure limits are checked in the pump hardware. Pressure checking doesn't start immediately after the pump is started, but with a few minutes delay. During this delay the pressure in chromatographic system can stabilize.

Max. Pressure for Set Flow

Sets the maximum pressure to be used in the *Set Flow* dialog in the [Device Monitor](#). Initial value is 1 MPa.

Solvent 1 (.4)

It is possible to enable/disable particular solvent, as well as to set custom name to it.

4.3 Method Setup - LC

This tab defines the properties of the **Flom UI-22 series** or **Flom UI-32 series** pump set as auxiliary.

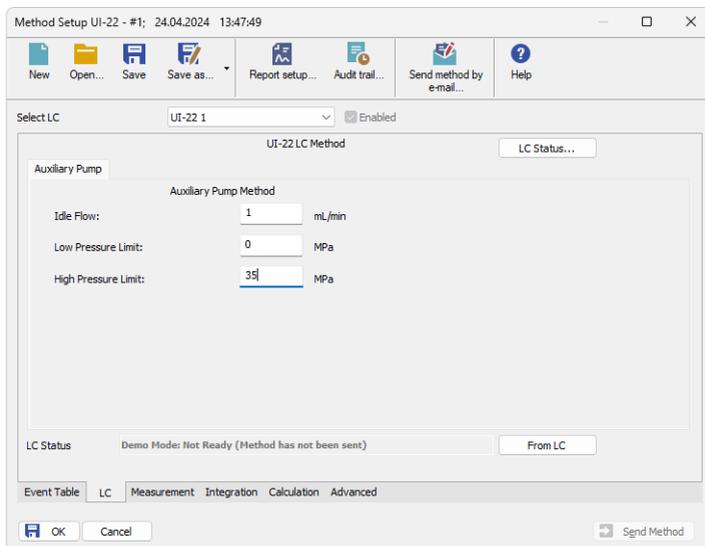


Fig. 8: Method Setup - LC - Auxiliary Pump

Idle Flow

Sets the flow of the pump used outside of the run. The flow of the pump that should be used during the run can be defined in the *Event Table*.

Low Pressure Limit

Sets the minimum pressure for the given auxiliary pump. When pressure reaches the set value, the pump will shut down. This prevents the solvent leakage. The range for *Min. Pressure* values is dependent on the pump variant and used pump head.

High Pressure Limit

Sets the maximum pressure for the given auxiliary pump. When pressure reaches the set value, the pump will shut down. This serves to prevent the damage to the pump when the column is blocked. The range for *Max. Pressure* values is dependent on the pump variant and used pump head and is limited by the value set for the pressure in the [DataApex UNI Setup](#) dialog.

4.3.1 Hardware Configuration

The *Hardware Configuration* dialog (invoked by using the *LC Status* button from the *Method Setup - LC* dialog) displays the configuration of the **Flom UI-22 series** or **Flom UI-32 series** pump, namely the communication type and its parameters.

The screenshot shows a dialog box titled "Hardware Configuration" with a close button (X) in the top right corner. It contains the following fields and a table:

- Ruby Script:** A text field containing the path "Utils\Jni_Drivers\FLOM\FlomUI22Pumps.rb".
- Port:** A dropdown menu currently set to "COM1".
- Table:** A table with two columns: "Property" and "Value".

	Property	Value
1	LC Name	LC 1
2	Pump number	1
3	Do not Stop when Closing Instrument	<input type="checkbox"/>
4	Auxiliary Pump	<input checked="" type="checkbox"/>
5	Maximum High Pressure Limit [MPa]	35
6	Maximum flow [ml]	10

At the bottom of the dialog, there are two buttons: "Close" and "Help".

Fig. 9: Hardware Configuration

4.4 Method Setup - Event Table

The *Method Setup - Event Table* tab allows the control of the **Flom UI-22 series** or **Flom UI-32 series** pump set as auxiliary pump during a run and enables switching of the auxiliary output.

Note: It is not possible to switch auxiliary output or change flow on a pump that is part of the gradient from the **Event Table**.

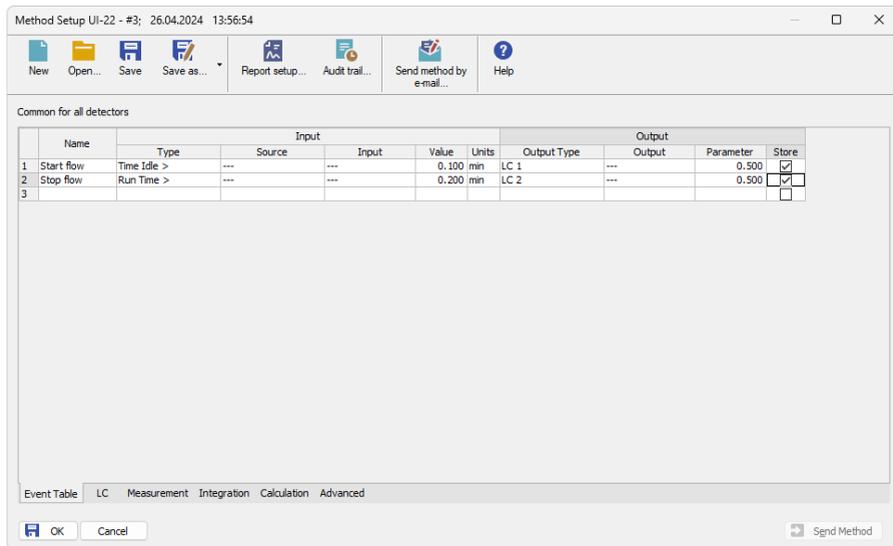


Fig. 10: Method Setup - Event Table

4.5 Method Setup - Aux. Signals

The *Method Setup - Aux Signals* tab serves for setting the usage of auxiliary signals of the **Flom UI-22 series** or **Flom UI-32 series** pump.

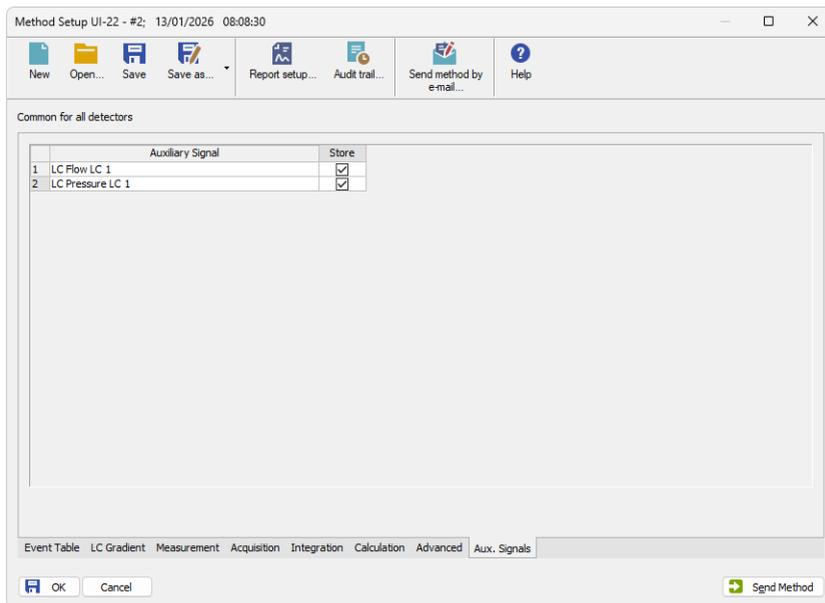


Fig. 11: Method Setup - Aux Signals

The list of available auxiliary signals is shown in the table in the dialog. By checking the checkbox in the *Store* column for the particular row, the given auxiliary signal will be stored into the measured chromatogram.

4.6 Device Monitor

The window with the pump status can be invoked by the *Analysis - Device Monitor* command from the *Instrument* window or using the *Device Monitor* icon .

Device Monitor - LC Monitor

For gradient pumps, the monitor consists of the section common to all pumps present in the gradient.

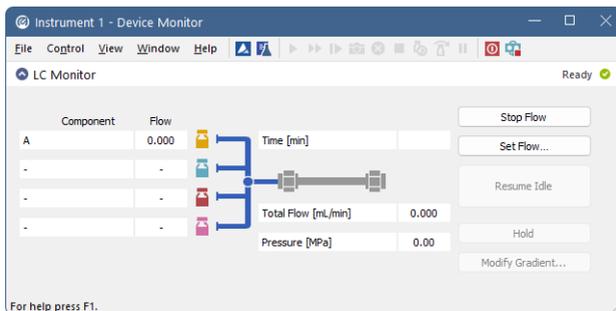


Fig. 12: Pump - Device Monitor

Stop Flow

The pumps can be stopped from this window using the *Stop Flow* button. This action will stop the pump only, the analysis run will continue and must be stopped or aborted separately by the *Stop/Abort* button in the toolbar.

Set Flow

Sets the desired total flow and solvent ratios in the opened *Set Flow* dialog. *Max. Pressure* sets the maximum pressure to be used. Initial value is 1 MPa.




Fig. 13: Set Flow

Resume Idle

Returns the pumps to *IDLE* state as defined in the appropriate field on the *LC Gradient* tab of the *Method Setup* dialog.

Hold/Resume

Clicking on the *Hold* button will keep the current gradient conditions until *Resume* is clicked.

Modify Gradient...

Opens the [LC Control Manual Flow](#) dialog allowing to set custom flow and mobile phase composition, disregarding the **Gradient Table** set in the method. The command is only available during the analysis run.

Device Monitor - Auxiliary Pump

Each Auxiliary pump has its own device monitor displaying the actual flow and pressure on the device. This separate monitor mimics the operations of *Stop Flow*,

Purge and *Resume Idle* from the gradient *Device Monitor*, but can also be used during the analysis run.

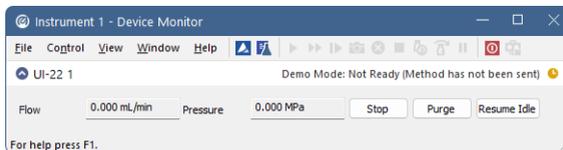


Fig. 14: Device Monitor - Auxiliary pump

Note: Please note that the separate *Purge* dialog is present for each auxiliary pump. Auxiliary pumps must thus be purged manually one at a time.




Fig. 15: Purge - Auxiliary pump

4.6.1 LC Control Manual Flow

The *LC Control Manual Flow* dialog accessible through using the *Modify Gradient ...* button from [Device Monitor](#) window allows the user to set a custom mobile phase composition and flow while the analysis is running. It resembles the [Method Setup - LC Gradient](#) tab in functionality.



Fig. 16: LC Control Manual Flow dialog

The *LC Control Manual Flow* dialog is only available during the analysis run. When it is invoked and the **OK** button is pressed, the original **Gradient Table** from the

acquisition method is discarded and replaced by the **Gradient Table** from the *LC Control Manual Flow* dialog. Any such operation is recorded in the audit trail of the measured chromatogram.

Caution: After the analysis run which used manual flow changes ends, the original method is automatically sent to all controlled devices to make sure **Clarity** station returns to the original method.

5 Report Setup

The pump section on the method report can be enabled by checking the *Instrument Control* checkbox on the *Method* tab of the *Report Setup* dialog.

The screenshot shows a 'Print Preview' window with the following content:

Standby Flow : 1.00 mL/min
 Time to Standby : 0.00 min
 Min. Pressure : 0.00 MPa

Idle State : Initial
 Standby Time : 0.00 min
 Max. Pressure : 35.00 MPa

Gradient Table

Time [min]	A [%]	B [%]	C [%]	Flow [mL/min]
Initial	80	18	2	1.000
8.00	80	18	2	1.000
15.00	60	38	2	1.000
20.00	20	78	2	1.000
27.50	20	78	2	1.000

Auxiliary Signal

Signal Name	Stored
LC Flow LC 1	<input type="checkbox"/>
LC Pressure LC 1	<input type="checkbox"/>
LC Flow LC 2	<input type="checkbox"/>
LC Pressure LC 2	<input type="checkbox"/>
LC Flow LC 3	<input type="checkbox"/>
LC Pressure LC 3	<input type="checkbox"/>

Configuration

Property	Value
LC Name	LC 1
Pump number	1
Do not Stop when Closing Instrument	<input type="checkbox"/>
Auxiliary Pump	<input type="checkbox"/>
Maximum High Pressure Limit [MPa]	35
Maximum Flow [mL]	10

Page 1

Fig. 17: Report Setup

All of the parameters set in the *Method Setup - LC Gradient* dialog are reported, as well as the custom *Pump Name* and other parameters set in the *DataApex UNI Setup* dialog. If the pump is configured as an Auxiliary Pump, the parameters set in the *Method Setup - LC* dialog are reported instead.

6 Troubleshooting

When the solution to a problem cannot be found easily, a recording of the communication between Clarity and the pump will significantly help DataApex support. The data recording can be enabled by adding or amending the COMMDRV.INI file in the Clarity installation directory (C:\CLARITY\CFG by default). The file can be edited in any text editor (e.g. Notepad). The following section should be edited or added:

```
[COM1]
echo=on
textmode=on
filename=CommDrvCOM1_%D.txt
reset=off
```

Note: Instead of COM1, type the communication port used to communicate with the **Flom UI-22 series** or **Flom UI-32 series** pump. This port number is displayed when the *LC Status* button in the [Method Setup - LC](#) dialog is invoked.

Note: %D (or %d) in the filename parameter means that the log will be created separately for each day. The *reset=off* parameter disables deleting the content of the log each time the station is started during the same day.

The created *.TXT files will be of great help in the diagnosis of not documented errors and communication issues.